


Post-operative oedema prevention

Preventing the build-up of post-operative oedema following total hip replacement surgery.


An RCT comparing the effectiveness of the gekoTM device to compression stockings in preventing the formation of oedema following total hip replacement surgery on the operated leg¹.

[Link to paper](#)

A feasibility randomised controlled trial to evaluate the effectiveness of a novel neuromuscular electro-stimulation device in preventing the formation of oedema following total hip replacement surgery

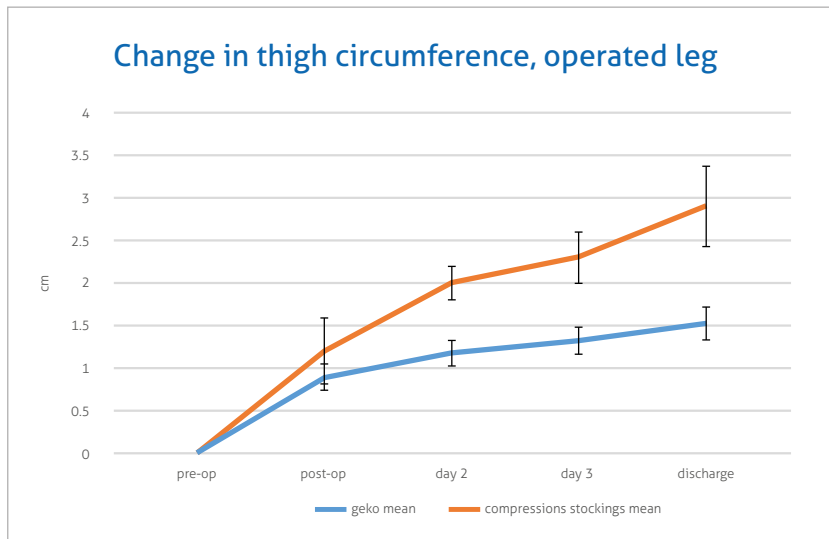

Mechanism of action animation video:

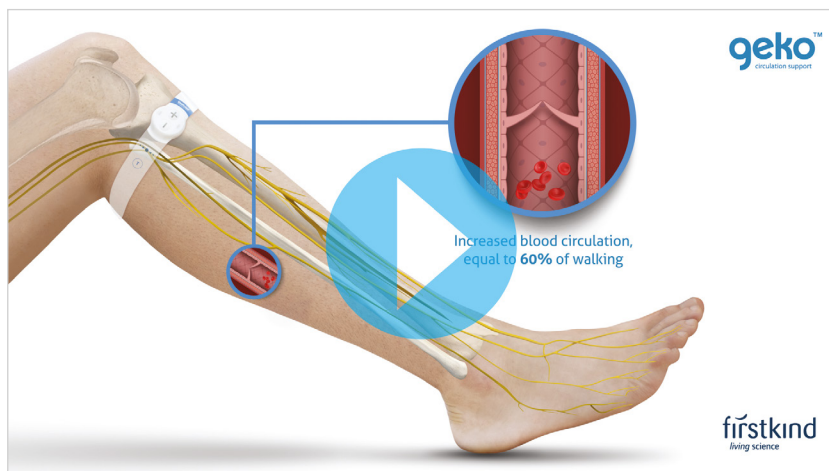

www.gekodevices.com

References:

1. Wainwright T W et al. Feasibility randomised controlled trial to evaluate the effectiveness of a novel neuromuscular electro-stimulation device in preventing the formation of oedema following total hip replacement surgery. Heliyon. 2018 Jul; 4(7): e00697. Published online 2018 Jul 18. doi: 10.1016/j.heliyon.2018.e00697.

